Important Steps When Using the A1CNow®+ System

Review A1CNow+ Professional Procedure Guide insert for full testing instructions before using this abbreviated guide.

A1CNow®+ SYSTEM

1 Preparing to test — Match lot numbers and open Pouch 1*

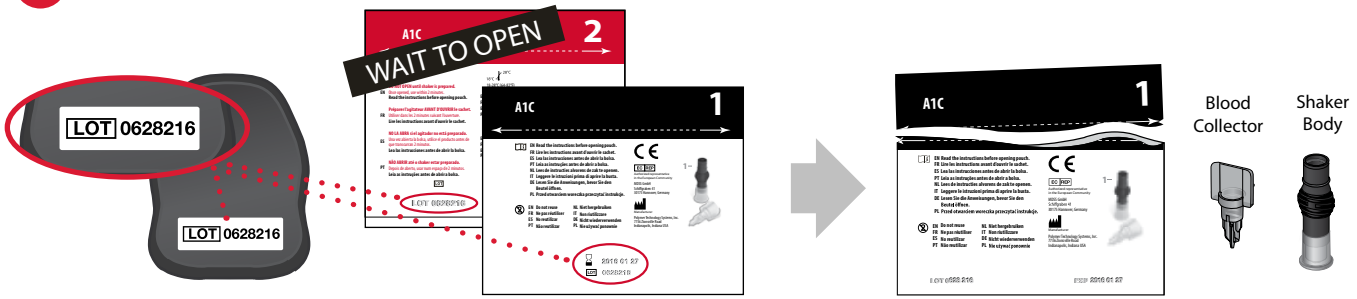

IMPORTANT:
Do not open *Pouch 2* until *Step 3* as shown below

2 Collecting the right amount of blood

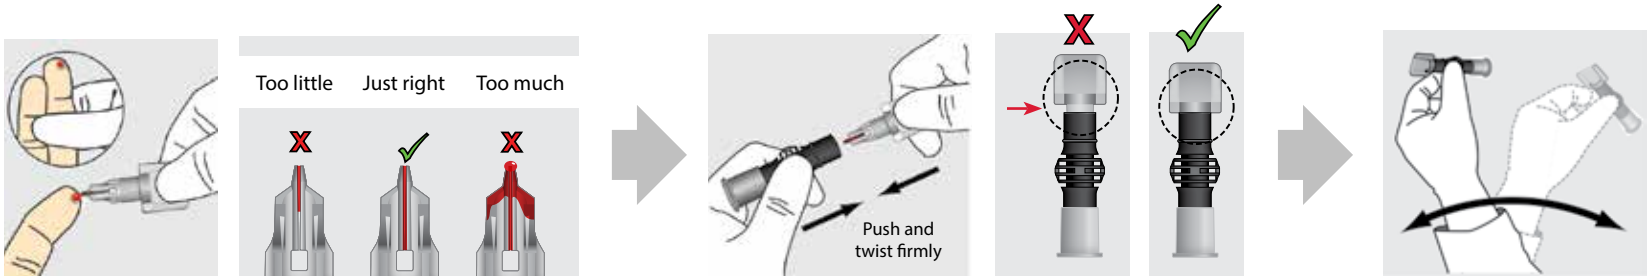

Gently touch blood drop to fill

Insert blood collector all the way into shaker body

Shake well 6-8 times

3 Open Pouch 2*. Insert cartridge, wait for SMPL to appear and dispense sample

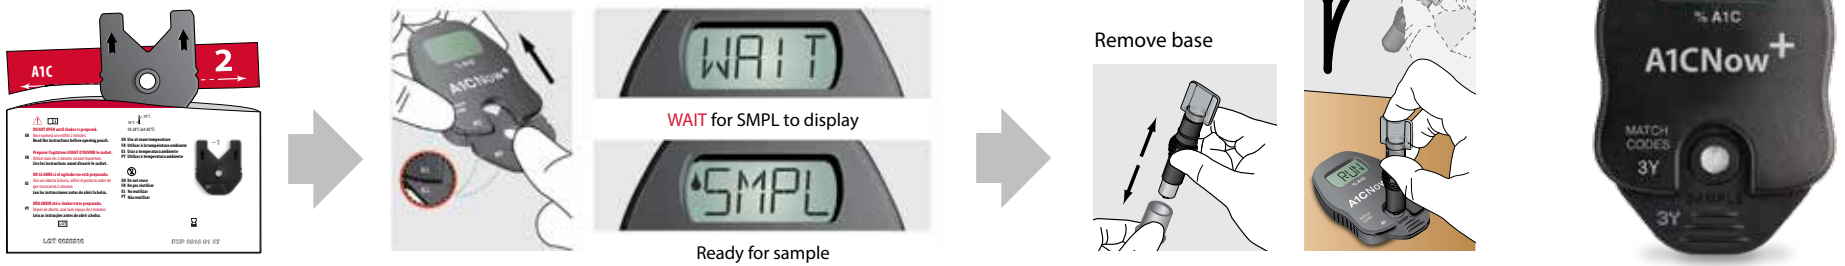

WAIT for SMPL to display

Ready for sample

Do not handle the analyzer until test is complete; results in 5 minutes

* Pouch illustrations may vary.

A1CNow is a trademark of Polymer Technology Systems, Inc. ©2018 Polymer Technology Systems, Inc. LIT001664 EN Rev. 2 01/18