iSCREEN™

# URINE TEST

## DX DRUG SCREEN SQUARE CUP

PROCEDURE CARD

Product Categorization as CLIA WAIVED

For detailed instructions, please read the package insert. Intended for *in vitro* diagnostic use.

## Kit Contents

25 iSCREEN™ Urine Test Dx Drug Screen Square Cups
One (1) Package Insert
One (1) Procedure Card
One (1) Adulteration Color Comparison Chart (If equipped)
25 Security Seals

*Store at 4°C-30°C (39°F-86°F) in the original sealed pouch. Do not freeze.*

## Cup Components




## Collection and Testing Procedure

**1** *Collect specimen and attach lid.*

**2** *Verify the urine temperature is within acceptable range of 32°C-38°C (90°F-100°F).*

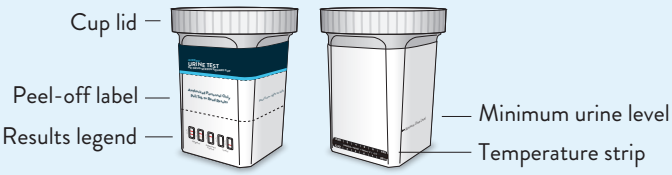


*Read the temperature strip within 2-4 minutes after urine is voided into the cup, verify the urine temperature is within the acceptable range.*

**3** *Peel off label to reveal results.*

*If applicable, read adulteration test results immediately, or at 30 seconds, or at 45 seconds (See package insert).*

Adulteration test results

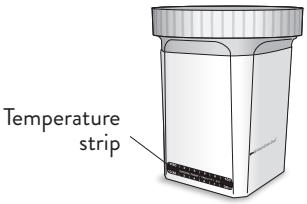

Adulteration on test result (If applicable)

*If the cup is equipped with adulterant pads, verify that pad colors are within acceptable range according to the adulteration color comparison chart.*



*For illustrative purposes only. Please refer to adulteration color comparison chart included with kit.*

*Adulteration color comparison chart*

**4** *Wait 5 minutes and read drug test result.*




Drug test result interpretation




## Laboratory Confirmation

Preliminary positive drug test results

*Apply security seal to preliminary positive specimen being sent for lab confirmation.*

Security seal

*This assay provides only a preliminary analytical test result. A more specific alternative chemical method must be used in order to obtain a confirmed analytical result. Gas chromatography-mass spectrometry (GC-MS) and liquid chromatography-tandem mass spectrometry (LC-MS/MS) are the preferred confirmatory methods. Clinical consideration and professional judgment should be applied to any drug test result, particularly when preliminary positive results are indicated.*

Distributed by Instant Technologies, Inc. Portsmouth, VA 23704 USA
Made in China

© 2022 Abbott. All rights reserved. All trademarks referenced are trademarks of either the Abbott group of companies or their respective owners.

Rel.: 2022/10/27